


Successful removal of a migrated biliary plastic stent using a novel spiral dilator


OPEN
ACCESS

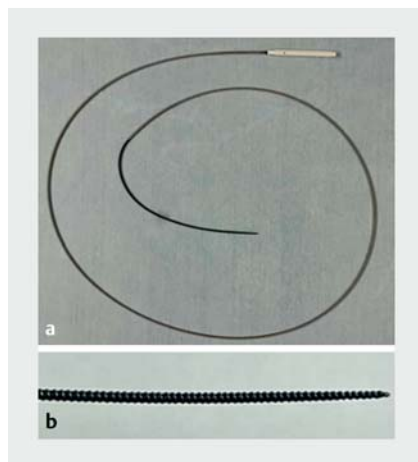


► **Fig. 1** Novel spiral dilator (Tornus ES). **a** The dilator is composed of a coil sheath and handle to rotate. The maximal outer diameter is 7 Fr. **b** The tip of the dilator is screw-shaped and tapered, allowing it to advance over the guidewire. There are two lines dedicated to 0.025- and 0.018-inch guidewires.

Endoscopic plastic stenting is an established biliary drainage technique. However, plastic stents may migrate proximally or distally, causing recurrent biliary obstruction [1]. The Tornus ES (Olympus Co., Tokyo, Japan) is a newly designed coil-sheath dilator with a screw-shaped tapered tip (► **Fig. 1**) that has been recently reported in endoscopic interventions [2–5]. We herein introduce successful troubleshooting using this novel spiral dilator for removal of a migrated biliary plastic stent.

A 63-year-old man presented with obstructive jaundice caused by pancreatic head cancer. Because he had undergone biliary drainage using an 8.5-Fr plastic stent with sphincterotomy 2 months before, we attempted to exchange the stent. The tumor had invaded the duodenum, and the plastic stent had almost migrated (► **Fig. 2**). We chose to use a novel spiral dilator (Tornus ES) because a 0.025-inch guidewire could be introduced into the stent. Its tip was inserted

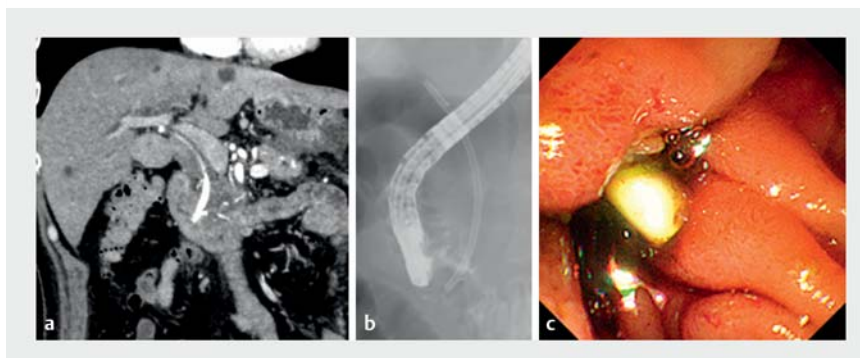

► **Fig. 2** A migrated biliary stent. **a** A computed tomography image showing pancreatic cancer and a plastic stent. Endoscopic biliary drainage had been performed using an 8.5-Fr plastic stent. The pancreatic cancer had invaded not only the distal bile duct but also the duodenum. **b** Fluoroscopic image revealed duodenal stricture around the periampullary area without gastric output obstruction. **c** Endoscopic image of the plastic stent, which had almost migrated into the bile duct.

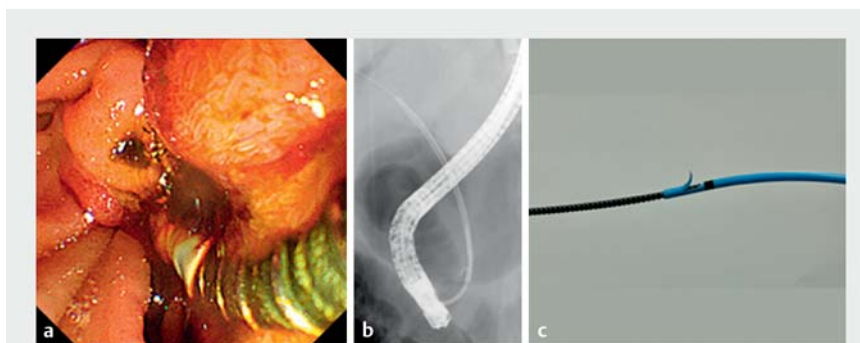


► **Fig. 3** Stent removal using the spiral dilator. **a** Endoscopic image showing that the spiral dilator was inserted into the distal end of the stent. **b** Fluoroscopic image showing that the spiral dilator was inserted into the distal end of the stent through the guidewire. **c** Ex vivo image of the spiral dilator and the same stent as the migrated stent. The spiral dilator and 8.5-Fr plastic stent are engaged.


into the distal end of the stent over the guidewire, and care was taken not to push the stent up (► **Fig. 3 a**). It was then advanced smoothly into the inside of the stent and spiral dilator were engaged, we confirmed that the stent rotated in accordance with the movement of the spiral dilator under endoscopic or fluoroscopic vision (► **Fig. 3 b**). Finally, the stent was successfully removed with the spiral

dilator through the scope channel (► **Fig. 3 c**, ► **Video 1**).

Although the outer diameter of the Tornus ES is 7 Fr, it could be inserted and engaged with 7-, 8.5-, and 10-Fr plastic stents in an ex vivo trial (► **Fig. 4 b, c, d**). In contrast, the tapered tip of the Tornus ES could not be inserted into a 6-Fr stent (► **Fig. 4 a**). Depending on the inner diameter of the stent, there is a high possibility that plastic stents of 7-Fr or

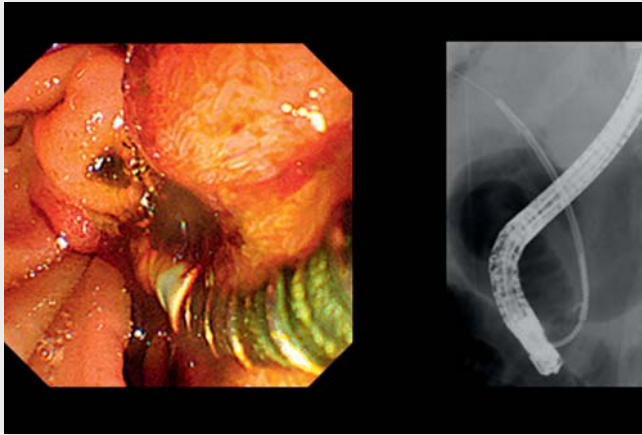

▶ Video 1 Endoscopic removal of a migrated biliary plastic stent using a novel spiral dilator.

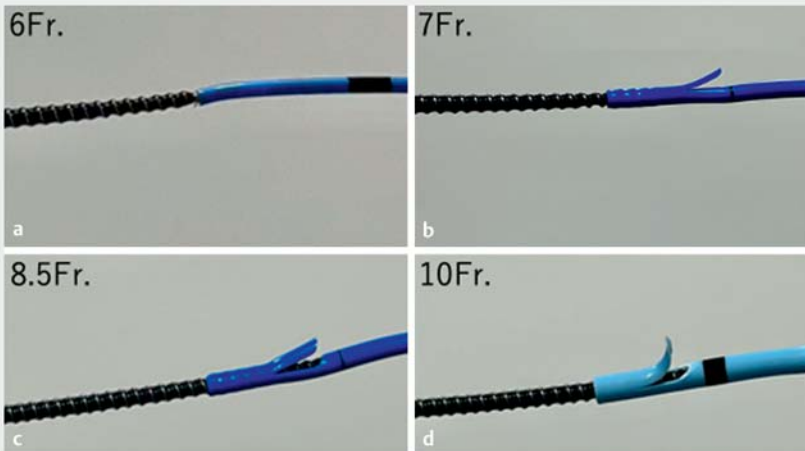

▶ Fig. 4 Ex vivo trial. **a** The spiral dilator cannot be inserted into and engaged with a 6-Fr stent. **b, c, d** The spiral dilator can be inserted and engaged with plastic stents of 7 Fr or larger.

larger can be removed. This case demonstrates that removal of a migrated plastic stent using Tornus ES can be a troubleshooting option.

Endoscopy_UCTN_Code_TTT_1AR_2AZ

Acknowledgments

We thank Angela Morben, DVM, ELS, from Edanz (<https://jp.edanz.com/ac>), for editing a draft of this manuscript.

Competing interests

The authors declare that they have no conflict of interest.

The authors

Yusuke Ishida¹, Takehiko Koga¹, Naoaki Tsuchiya¹, Kaori Hata², Kei Nishioka², Noriko Shiga², Fumihito Hirai¹

- 1 Department of Gastroenterology and Medicine, Fukuoka University, Faculty of Medicine, Fukuoka, Japan
- 2 Department of Gastroenterology, Fukuokaken Saiseikai Futsukaichi Hospital, Fukuoka, Japan

Corresponding author

Yusuke Ishida, MD

Department of Gastroenterology and Medicine, Fukuoka University, Faculty of Medicine, 7-45-1 Nanakuma, Jonan-ku, Fukuoka 814-0180, Japan
 Fax: +81 92 863 9759
 y.ishida.cb@fukuoka-u.ac.jp

References

- [1] Okabe Y, Tsuruta Y, Kaji Y et al. Endoscopic retrieval of migrated plastic stent into bile duct or pancreatic pseudocyst. *Dig Endosc* 2009; 21: 1–7
- [2] Yasuda T, Hara K, Haba S. Dilation of pancreatic duct stenosis using a newly designed drill dilator. *Dig Endosc* 2022; 34: e73–e74
- [3] Mandai K, Inoue N. Removal of biliary plastic stent using a novel spiral dilator for reliable stent placement. *Dig Endosc* 2022; 34: e168–e169
- [4] Yamada M, Hara K, Haba S et al. Endoscopic ultrasound-guided hepaticogastrostomy using a novel spiral dilator. *Endoscopy* 2022; 54: E856–E857
- [5] Yamada M, Okamoto T, Sasahira N. Troubleshooting with a drill dilator for the stent-in-stent technique in malignant hilar biliary obstruction. *Endoscopy* 2023; 55: E189–E190

Bibliography

Endoscopy 2023; 55: E804–E805
 DOI 10.1055/a-2098-0982
 ISSN 0013-726X
 © 2023. The Author(s).

This is an open access article published by Thieme under the terms of the Creative Commons Attribution License, permitting unrestricted use, distribution, and reproduction so long as the original work is properly cited.

(<https://creativecommons.org/licenses/by/4.0/>)

Georg Thieme Verlag KG, Rüdigerstraße 14, 70469 Stuttgart, Germany

