



Endoscopic ultrasound-guided hepaticojejunostomy for complete biliary anastomotic stricture: the echo-free space technique for scope insertion in surgically altered anatomy


OPEN
ACCESS

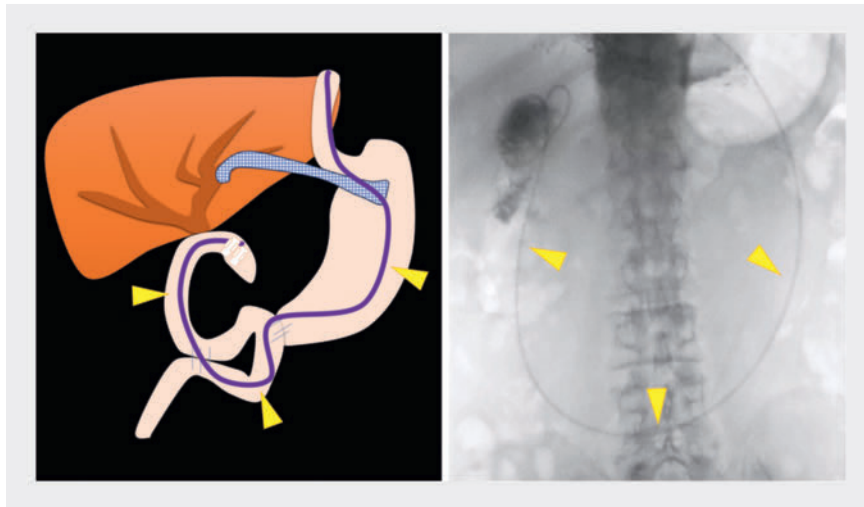

► **Fig. 1** Schematic diagram and fluoroscopic image showing a 6-Fr endoscopic nasobiliary drainage catheter (arrowheads) placed near the anastomotic stricture after a single-balloon enteroscope had been inserted up to the anastomosis, which was marked with a clip.

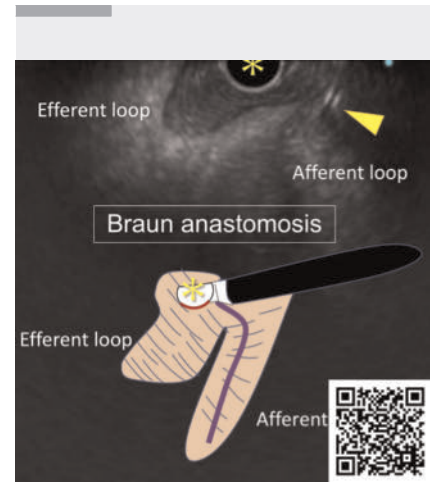

► **Video 1** Endoscopic ultrasound-guided hepaticojejunostomy is performed in a patient with complete biliary anastomotic stricture using the echo-free space technique to insert the scope into the choledochojejunostomy site.

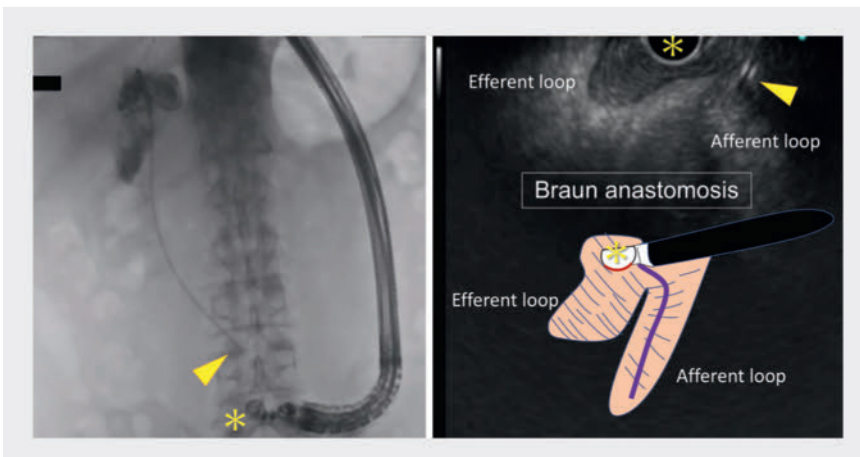

► **Fig. 2** A side-viewing linear endoscope (asterisk) is used to identify the Braun anastomosis, relying on careful observation of the echo image, the endoscopic nasobiliary drainage catheter (arrowhead) is used as a guide to reach the choledochojejunostomy.


Postoperative biliary strictures are estimated to occur in 2.6% of patients. When endoscopic treatment is difficult, they can be treated with endoscopic ultrasound-guided hepaticojejunostomy (EUS-HJS) using a forward-viewing linear endoscope [1–4]. However, in many institutions, the forward-viewing scope

is not readily available, making immediate intervention difficult. We have developed a safe and reliable method for inserting a side-viewing linear endoscope [5].


We present the case of a 71-year-old man who underwent total pancreatectomy

and choledochojejunostomy for pancreatic cancer. After 8 months, he developed cholangitis due to an anastomotic stricture and was referred to our department. Single-balloon endoscopic retrograde cholangiopancreatography (ERCP) and EUS-guided hepaticogastrostomy (EUS-HGS) were attempted, but the patient continued to have recurrent cholangitis. We therefore decided to perform EUS-HJS from the anastomotic site.


The single-balloon enteroscope was first inserted up to the anastomosis, which was marked with a clip; a 6-Fr endoscopic nasobiliary drainage (ENBD) catheter was placed near the anastomotic stricture (► **Fig. 1**). The scope was switched to a side-viewing linear endoscope (GF-UCT260) and the Braun anastomosis was identified on careful observation of the echo image, with the ENBD catheter used as a guide to reach the HJS (► **Fig. 2**; ► **Video 1**). The bile duct was punctured

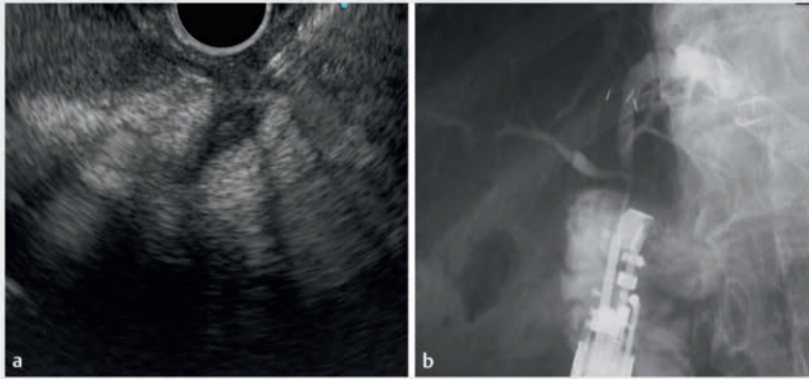

► **Fig. 3** Endoscopic ultrasound and fluoroscopic images showing: **a** the bile duct being punctured through the anastomosis using a 19G needle; **b** the appearance after the injection of contrast medium.

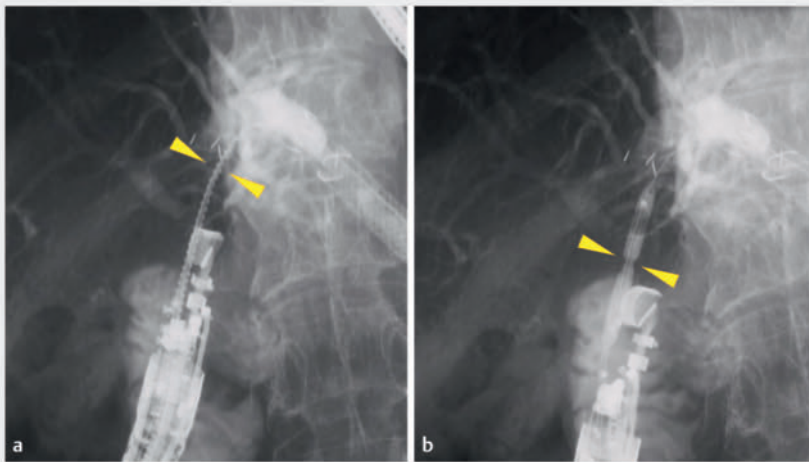

► **Fig. 4** Fluoroscopic images showing the stenosis being dilated with a spiral drill dilator and tapered-tip balloon catheter.

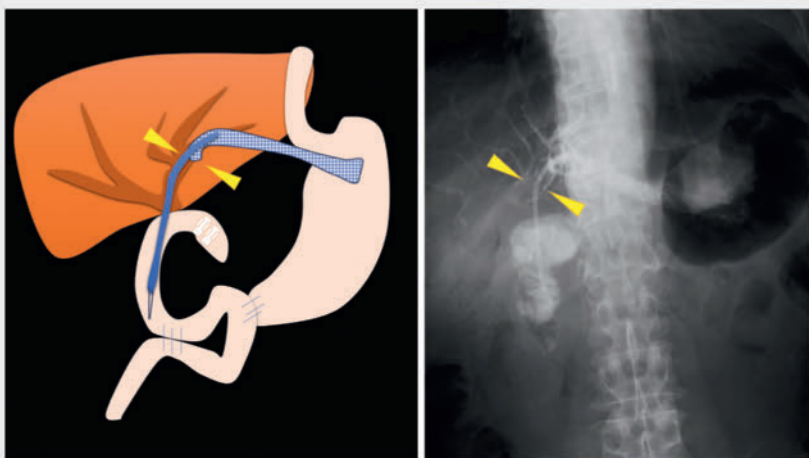

► **Fig. 5** Schematic diagram and fluoroscopic image showing a 7-Fr, 9-cm inside stent (arrowhead) placed to complete the procedure.

through the anastomosis with an 19G EZ Shot 3 Plus (Olympus) and a guidewire was placed (► **Fig. 3**). The stenosis was dilated with a spiral drill dilator (Tornus ES; Olympus) and then with a tapered-tip balloon catheter (REN; Kaneka) up to 4mm (► **Fig. 4**), and the procedure was completed with the placement of a 7-Fr, 9-cm inside stent (► **Fig. 5**).

This case suggests that the echo-free space technique using a side-viewing linear endoscope can be useful in post-operative patients and represents a new option for EUS-HJS in the treatment of complete biliary anastomotic stricture.

Endoscopy_UCTN_Code_TTT_1AS_2AH

Conflict of Interest

The authors declare that they have no conflict of interest.

The authors

Michihito Kono^{1,2}, **Shunsuke Omoto**³, **Mamoru Takenaka**³, **Akito Furuta**^{1,2}, **Shunsuke Ogata**^{1,2}, **Taro Inoue**^{1,2}, **Wataru Ono**^{1,2}

- 1 Gastroenterology, Kishiwada Tokushukai Hospital, Osaka, Japan
- 2 Gastroenterology, Kobe Tokushukai Hospital, Kobe, Japan
- 3 Gastroenterology and Hepatology, Kindai University Hospital, Osaka-Sayama, Japan

Corresponding author

Shunsuke Omoto, MD, PhD

Department of Gastroenterology and Hepatology, Kindai University Faculty of Medicine, 377-2 Ohno-Higashi, Osaka-Sayama, 589-8511, Japan
shunsuke.oomoto@gmail.com

References

- [1] House MG, Fong Y, Arnaoutakis DJ et al. Preoperative predictors for complications after pancreaticoduodenectomy: impact of BMI and body fat distribution. *J Gastrointest Surg* 2008; 12: 270–278. doi:10.1007/s11605-007-0421-7
- [2] Itoi T, Ikeuchi N, Tonozuka R et al. EUS-guided choledochojejunostomy with a lumen-apposing metal stent in a post-Whipple patient. *Gastrointest Endosc* 2015; 81: 1259–1260
- [3] Kida M, Yamauchi H, Okuwaki K et al. Endoscopic ultrasound-guided choledochojejunostomy with a forward-viewing echoendoscope for severe benign bilioenteric stricture in a patient with Child's resection. *Endoscopy* 2015; 47 (Suppl. 1): E303–E304
- [4] Koizumi K, Masuda S, Shionoya K et al. Endoscopic ultrasound-guided hepaticojejunostomy using forward-viewing echoendoscope for transected aberrant right posterior hepatic duct in Roux-en-Y hepaticojejunostomy. *Endoscopy* 2022; 54: E933–E934. doi:10.1055/a-1881-4068
- [5] Omoto S, Takenaka M, Fukunaga T et al. The “echo-free space” technique: a safe and reliable method for endoscopic ultrasound scope insertion. *Endoscopy* 2023; 55: E698–E699

Bibliography

Endoscopy 2024; 56: E706–E708

DOI 10.1055/a-2368-3932

ISSN 0013-726X

© 2024. The Author(s).

This is an open access article published by Thieme under the terms of the Creative Commons Attribution License, permitting unrestricted use, distribution, and reproduction so long as the original work is properly cited.

(<https://creativecommons.org/licenses/by/4.0/>)

Georg Thieme Verlag KG, Rüdigerstraße 14, 70469 Stuttgart, Germany



ENDOSCOPY E-VIDEOS

<https://eref.thieme.de/e-videos>



E-Videos is an open access online section of the journal *Endoscopy*, reporting on interesting cases

and new techniques in gastroenterological endoscopy. All papers include a high-quality video and are published with a Creative Commons CC-BY license. *Endoscopy E-Videos* qualify for HINARI discounts and waivers and eligibility is automatically checked during the submission process. We grant 100% waivers to articles whose corresponding authors are based in Group A countries and 50% waivers to those who are based in Group B countries as classified by Research4Life (see: <https://www.research4life.org/access/eligibility/>).

This section has its own submission website at <https://mc.manuscriptcentral.com/e-videos>