



Suprapapillary trisectoral deployment of slim fully covered metal stents with ultra-stiff high-sliding guidewires for malignant hilar biliary obstruction

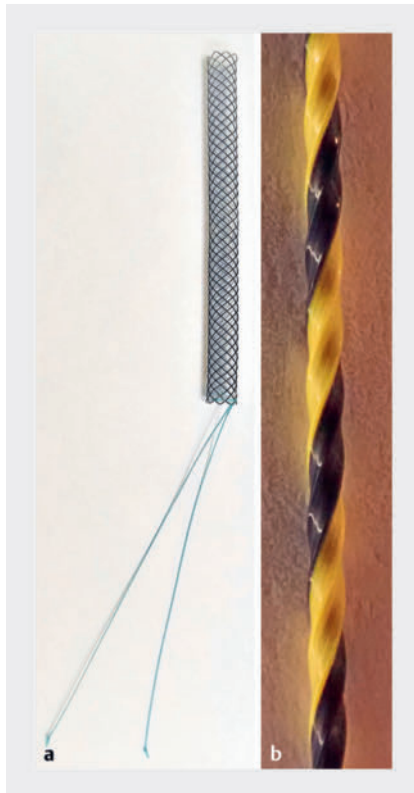

► **Fig. 1** Device images. **a** The slim, fully covered metal stent (Taewoong Medical, Seoul, Korea) has a diameter of 6 mm, incorporates a retrieval string at the distal end, and boasts a 7.5-Fr delivery system. **b** The novel 0.035-inch guidewire (Seek-Master Hard; Piolax Medical Devices, Kanagawa, Japan) has a thick, 0.7-mm, high-rigidity, nickel-titanium core with polytetrafluoroethylene coating that undergoes "ridge-processing" to minimize contact area and friction. This process improves the deliverability and trackability of the entire system.

Placement of bilateral suprapapillary uncovered metal stents is recommended for unresectable malignant hilar biliary obstruction (MHBO) owing to superior patency compared with plastic stents, unilateral placement, and positioning across the papilla [1–3]. Recent studies also suggest that bilateral trisectoral

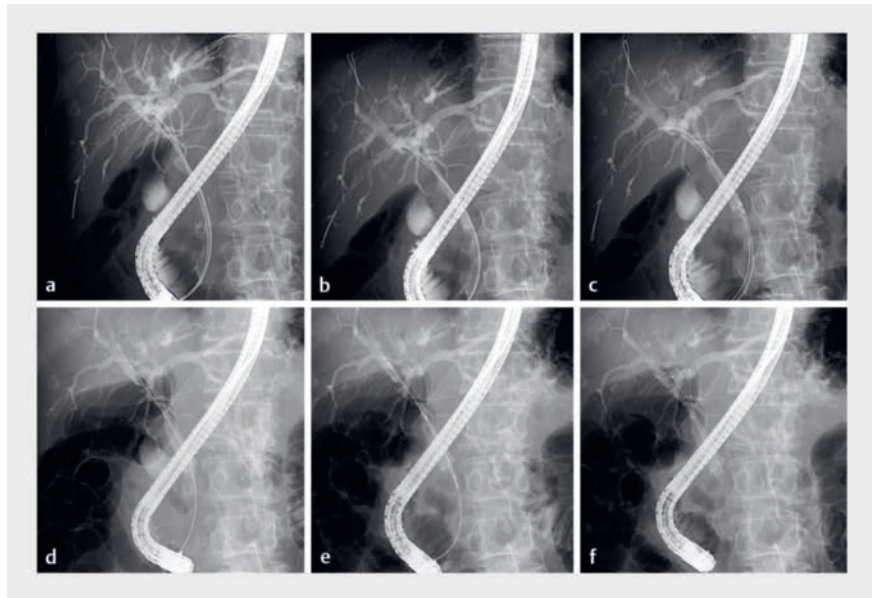


► **Fig. 2** Fluoroscopic images. **a** Three novel, ultra-stiff, high-sliding guidewires were placed into the right posterior, right anterior, and left hepatic ducts, respectively. **b** The delivery system of the first slim, fully covered metal stent was introduced over the left guidewire and deployed across the stricture and above the papilla. **c** The second metal stent was then inserted over the posterior guidewire. **d** The second stent was deployed alongside the left metal stent. **e** Finally, the third metal stent was inserted over the anterior guidewire. **f** The third stent was deployed in a stent-by-stent configuration.

placement further improves survival, especially in patients undergoing chemotherapy [4]. However, stent occlusion still affects approximately half of all cases, and reintervention for occlusion is technically demanding after bilateral placement of uncovered metal stents. Therefore, we proposed a novel approach, suprapapillary trisectoral placement of a slim, fully covered metal stent, which reduces the risk of side-branch occlusion and is easily removable, facilitating straightforward reintervention. Although insertion of the second and third stents becomes primarily challenging with this method, utilizing an ultra-stiff, high-sliding guidewire can circumvent this issue (► **Fig. 1**). The metal stent is 6 mm in diameter, incorporates a retrieval string at the distal

end, and boasts a 7.5-Fr delivery system. The novel 0.035-inch guidewire features a 0.7-mm high-rigidity, nickel-titanium core with polytetrafluoroethylene coating. Notably, this coat undergoes "ridge-processing" to minimize contact area and friction, thereby improving the deliverability and trackability of the entire system.

An 88-year-old man presented with obstructive jaundice due to Bismuth type IIIa MHBO. After placing three novel guidewires into the right posterior, right anterior, and left hepatic ducts, respectively, the delivery system of the stent was introduced over the left guidewire and deployed across the stricture and above the papilla. The second metal stent was subsequently inserted over the posterior guidewire and deployed

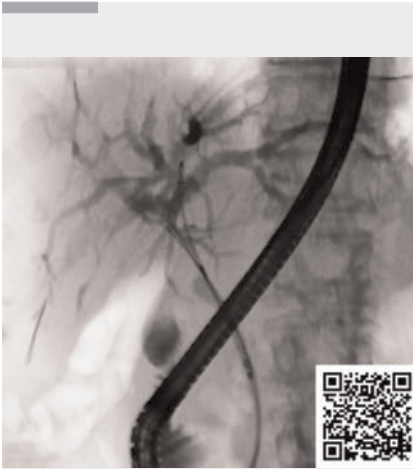

▶ Video 1 Suprapapillary trisectoral deployment of slim, fully covered metal stents with ultra-stiff, high-sliding guidewires for malignant hilar biliary obstruction.

alongside the left metal stent. Finally, the third metal stent was introduced over the anterior guidewire and deployed in a stent-by-stent configuration (▶ **Fig. 2**, ▶ **Video 1**). All three retrieval strings were positioned through the duodenal papilla. No adverse events or stent dysfunction occurred until the patient's death.

Overall, suprapapillary trisectoral placement of slim, fully covered metal stents shows potential as an uncomplicated and advantageous procedure for MHBO.

Endoscopy_UCTN_Code_TTT_1AR_2AZ

Conflict of Interest

The authors declare that they have no conflict of interest.

The authors

Tadahisa Inoue¹, Rena Kitano¹, Tomoya Kitada¹, Kazumasa Sakamoto¹, Satoshi Kimoto¹, Jun Arai¹, Kiyooki Ito¹

¹ Department of Gastroenterology, Aichi Medical University, Nagakute, Japan

Corresponding author

Tadahisa Inoue, MD, PhD

Department of Gastroenterology, Aichi Medical University, 1-1 Yazakokarimata, Nagakute, Aichi 480-1195, Japan
tinoue-tag@umin.ac.jp

References

- [1] Lee TH, Kim TH, Moon JH et al. Bilateral versus unilateral placement of metal stents for inoperable high-grade malignant hilar biliary strictures: a multicenter, prospective, randomized study (with video). *Gastrointest Endosc* 2017; 86: 817–827
- [2] Xia MX, Pan YL, Cai XB et al. Comparison of endoscopic bilateral metal stent drainage with plastic stents in the palliation of unresectable hilar biliary malignant strictures: large multicenter study. *Dig Endosc* 2021; 33: 179–189
- [3] Naitoh I, Inoue T. Optimal endoscopic drainage strategy for unresectable malignant hilar biliary obstruction. *Clin Endosc* 2023; 56: 135–142. doi:10.5946/ce.2022.150
- [4] Uchida D, Kato H, Muro S et al. Efficacy of endoscopic over 3-branched partial stent-in-stent drainage using self-expandable metallic stents in patients with unresectable hilar biliary carcinoma. *J Clin Gastroenterol* 2015; 49: 529–536

Bibliography

Endoscopy 2024; 56: E996–E997

DOI 10.1055/a-2452-5261

ISSN 0013-726X

© 2024. The Author(s).

This is an open access article published by Thieme under the terms of the Creative Commons Attribution License, permitting unrestricted use, distribution, and reproduction so long as the original work is properly cited.

(<https://creativecommons.org/licenses/by/4.0/>)

Georg Thieme Verlag KG, Oswald-Hesse-Str. 50, 70469 Stuttgart, Germany



ENDOSCOPY E-VIDEOS

<https://eref.thieme.de/e-videos>



E-Videos is an open access online section of the journal *Endoscopy*, reporting on interesting cases and new techniques in gastroenterological endoscopy. All papers include a high-quality video and are published with a Creative Commons CC-BY license. *Endoscopy E-Videos* qualify for HINARI discounts and waivers and eligibility is automatically checked during the submission process. We grant 100% waivers to articles whose corresponding authors are based in Group A countries and 50% waivers to those who are based in Group B countries as classified by Research4Life (see: <https://www.research4life.org/access/eligibility/>).

This section has its own submission website at <https://mc.manuscriptcentral.com/e-videos>