




# Comparison of Manual Two-dimensional and Automated Three-dimensional Methods of Assessing Shoulder Joint Morphology through Computed Tomography Images

## *Comparação de métodos bidimensionais manuais e tridimensionais automatizados de avaliação da morfologia da articulação do ombro por imagens de tomografia computadorizada*

Geraldo da Rocha Motta Filho<sup>1,2</sup>  Marcus Vinícius Amaral<sup>1,2</sup> Márcio Cohen<sup>1</sup>  
Marcio Schiefer de Sá Carvalho<sup>1</sup> Raphael Soares da Fonseca<sup>1</sup> Ana Carolina Leal de Oliveira<sup>3</sup>

<sup>1</sup>Shoulder and Elbow Surgery Center, Instituto Nacional de Traumatologia e Ortopedia, Rio de Janeiro, RJ, Brazil

<sup>2</sup>Division of Traumatology and Orthopedics (DITRO), Instituto Nacional de Traumatologia e Ortopedia, Rio de Janeiro, RJ, Brazil

<sup>3</sup>Teaching and Research Division, Instituto Nacional de Traumatologia e Ortopedia, Rio de Janeiro, RJ, Brazil

Address for correspondence Geraldo da Rocha Motta Filho, MD, MSc, Rua Raimundo de Magalhães 92, 22451-150, Rio de Janeiro, RJ, Brazil (e-mail: geraldomotta@terra.com.br).

Rev Bras Ortop 2024;59(4):e590–e598.

### Abstract

**Objective** To evaluate the interobserver agreement in the measurement of anatomical parameters of the shoulder using manual methods of two-dimensional (2D) computed tomography (CT) unformatted in the plane of the scapula and to compare them with the automated measurement obtained through the Blueprint (Wright Medical, Memphis, TN, United States) software, which uses reconstructed three-dimensional (3D) images.

**Methods** The present is a cross-sectional study in which 2D CT images of 38 patients with different diagnoses were used. The anatomical parameters were measured by the manual methods described by Friedman et al., the glenoid vault method, the Maurer et al. method, and shoulder subluxation according to Walch et al., by five independent qualified surgeons and compared with the parameters obtained through the Blueprint automated software.

**Results** Significant differences were found between the manual measurement version obtained through the Friedman et al. method and the automated version.

### Keywords

- ▶ arthroplasty
- ▶ shoulder replacement
- ▶ tomography, X-ray computed

Work carried out at the Shoulder and Elbow Surgery Center, Instituto Nacional de Traumatologia e Ortopedia, Rio de Janeiro, RJ, Brazil.

received  
September 22, 2023  
accepted  
April 5, 2024  
article published online  
July 8, 2024

DOI <https://doi.org/10.1055/s-0044-1786821>.  
ISSN 0102-3616.

© 2024. The Author(s).

This is an open access article published by Thieme under the terms of the Creative Commons Attribution 4.0 International License, permitting copying and reproduction so long as the original work is given appropriate credit (<https://creativecommons.org/licenses/by/4.0/>).

Thieme Revinter Publicações Ltda., Rua do Matoso 170, Rio de Janeiro, RJ, CEP 20270-135, Brazil

The mean values found for inclination did not show statistically significant differences among the methods. The mean value found for subluxation showed significant differences between the average observed in the analyses performed by the automated method and those performed by the surgeons.

**Conclusion** The manual measurements of glenoid version and inclination performed by experienced surgeons are effective, and the vault method is superior to the Friedman et al. method in the analysis of severe glenoid deformities.

## Resumo

**Objetivo** Avaliar a concordância interobservador na medida dos parâmetros anatômicos do ombro utilizando métodos manuais de tomografia computadorizada (TC) bidimensional (2D) não formatada no plano da escápula e compará-los à medida automatizada obtida com o programa Blueprint (Wright Medical, Memphis, TN, Estados Unidos), que utiliza imagens tridimensionais (3D) reconstruídas.

**Métodos** Este é um estudo transversal com a utilização de imagens de TC 2D de 38 pacientes com diferentes diagnósticos. Os parâmetros anatômicos foram medidos pelos métodos manuais descritos por Friedman et al., o método de *vault* glenoidal, o de Maurer et al. e o de subluxação do ombro segundo Walch et al. por cinco cirurgiões qualificados e independentes, e comparados aos parâmetros obtidos pelo programa automatizado Blueprint.

**Resultados** Foram observadas diferenças significativas entre a versão de medida manual obtida pelo método de Friedman et al. e a versão automatizada. Os valores médios de inclinação não apresentaram diferenças estatisticamente significativas entre os métodos. A média observada de subluxação teve diferenças significativas entre as análises realizadas pelo método automatizado e pelos cirurgiões.

**Conclusão** As medidas manuais de versão e inclinação da glenoide realizadas por cirurgiões experientes são eficazes, e o método da abóbada é superior ao de Friedman et al. na análise de deformidades glenoidais graves.

## Palavras-chave

- ▶ artroplastia
- ▶ substituição do ombro
- ▶ tomografia computadorizada por raios X

## Introduction

Correction of joint deformities in the glenoid is essential to perform shoulder arthroplasty, and it can directly impact the functional result and survival of the implant.<sup>1</sup> Therefore, preoperative planning is essential for the successful performance of total shoulder arthroplasty.<sup>1-4</sup>

Traditionally, the assessment of glenoid morphology is performed using angular measurements on two-dimensional (2D) computed tomography (CT) images, which have demonstrated low accuracy and inter- and intraobserver agreements.<sup>5</sup> The use of three-dimensional (3D) CT images has shown limited improvements as the reconstruction of the scapula plane requires reformatting and processing of 2D images.<sup>6,7</sup>

Thus, the emergence of three-dimensional (3D) CT images associated with the development of automated computer software is intended to control the limitations and inaccuracies of manual methods and the reformatting of CT slices in the scapular plane.<sup>8-11</sup>

Therefore, the aim of the present study was to evaluate the interobserver agreement in the measurement of anatomical parameters of the shoulder using manual methods from 2D CT unformatted in the plane of the scapula and to compare

them with automated measurement that uses reconstructed 3D images.

## Materials and Methods

### Selection of Cases

After approval by the institutional Ethics in Research Committee (under no. 35243920.4.0000.5273), a study was carried out to evaluate the CT images of the shoulder joint in patients of both sexes, older than 18 years of age, diagnosed with osteoarthritis.

In total, 38 CT scans were randomly selected from exams performed for patients at the institution from January 2015 to December 2019. All CT exams were performed using the same device (model Brilliance, Philips, Amsterdam, Netherlands), with 64 channels, with the patient in the supine position.

The inclusion criteria were CT scans that had triplanar, coronal, sagittal, and axial sections, with a minimum section thickness of 1 mm, in which the entire scapula was visualized and were processed by the automated surgical planning software selected for the experiment. Images of patients who had undergone previous surgery in the shoulder and who had artifacts on CT images were excluded, such as the presence of a metallic implant or other anatomical changes

that could affect the segmental processing by the automated software.

### Manual Measurement

The 2D CT images that were not formatted in the scapula plane were used for the manual measurement of the version, according to the Friedman et al.<sup>12</sup> (►Fig. 1) and glenoid vault methods, described by Matsumara et al.<sup>13</sup> (►Fig. 2), and of the glenoid inclination using the Maurer et al.<sup>14</sup> (►Fig. 3) method in addition to the measurement of the percentage of humeral head subluxation according to Walch et al.<sup>4</sup> (►Fig. 4).

These measurements were performed independently by five orthopedists specialized in shoulder surgery using the RadiAnt DICOM Viewer software (Medixant, Poznan, Poland).<sup>15</sup> The observers were uniformly instructed, as described below, to standardize the measurements. All observers were blinded to each other's results.


### Automated Measurement

The automated measurement used the CT images in the Digital Imaging and Communications in Medicine (DICOM) format that were processed by the Blueprint<sup>9</sup> (Wright Medical, Memphis, TN, United States) software. The software performs an automatic segmentation process, determines the scapula and glenoid planes, and then performs measurements, providing the version and inclination values, in addition to the percentage of subluxation of the humeral head (►Fig. 5).

### Statistical Analysis

The interclass correlation coefficient (ICC) was calculated to determine the variability in the manual measurements among surgeons.

For the descriptive statistics, data were presented as mean, standard deviation, maximum, and minimum values. The

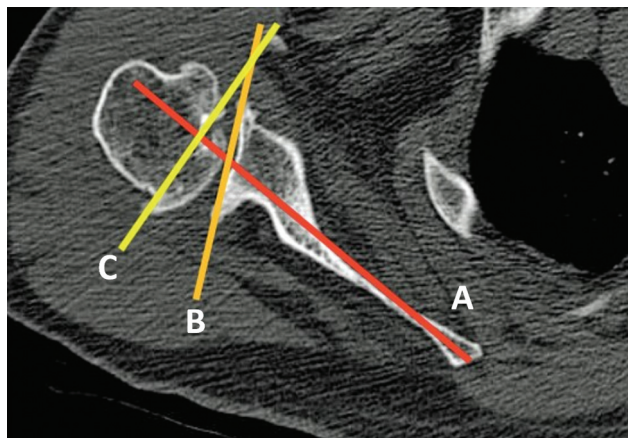

**Fig. 1** Friedman et al.<sup>12</sup> method to evaluate the glenoid version. We used the fourth cut distal to the last cut in which the tip of the coracoid process was visualized in the axial plane. The glenoid version was determined by the angle, as shown: (A) Friedman et al.<sup>12</sup> line, (B) glenoid line, and (C) line perpendicular to the scapular axis. A positive value of the glenoid version angle was interpreted as anteversion, while a negative value was interpreted as retroversion.

comparison of the measurements obtained by the different methods of evaluating the version was performed using the Friedman et al.<sup>12</sup> test, followed by the Dunn posttest. The comparison between the measurements of inclination and subluxation by manual and automated methods was performed using the Wilcoxon test. The cases were categorized according to the severity of the version and inclination, using intervals of 0 to 10°, and > 10° when indicated. Those intervals were chosen based on studies that have shown that the normal glenoid version is close to 0°, sometimes with slight anteversion but more often slight retroversion with values typically lower than 10° in either direction,<sup>16</sup> and that the normal intrinsic glenoid inclination angle is generally between 0 and 10°.<sup>17</sup> All analyses were performed using the IBM SPSS Statistics for Windows (IBM Corp., Armonk, NY, United States) software, version 21.0.

## Results

The present study included 38 cases, 17 of which were diagnosed with cuff tear arthropathy, and 21, with osteoarthritis.

The ICC for the manual measurements is described in ►Table 1. The mean version values obtained by the Friedman et al.,<sup>12</sup> vault, and automated methods are presented in ►Table 2. The vault method was similar to the automated method ( $p > 0.99$ ), while the Friedman et al.<sup>12</sup> method tended to underestimate this measure, both in relation to the automated and vault methods ( $p = 0.003$ ) (►Table 2).


The differences between the version measurements made by Blueprint and the Friedman et al.<sup>12</sup> method were lower than 5° in 23 cases (60.5%), between 5 and 10° in 14 cases (36.8%), and greater than 10° in 1 case (2.6%). Such proportions were similar to those found in the comparison between Blueprint and the vault method: 22 cases (57.8%), 13 cases (34.2%), and 3 cases (7.8%), respectively ( $p = 0.57$ ) (►Table 3).

Inclination showed no statistical difference between the automated and manual methods ( $11.85^\circ \pm 9.8^\circ$  versus  $11.24^\circ \pm 5.44^\circ$ ;  $p = 0.377$ ) (►Table 4). Subluxation measurements resulted in higher values in the automated method in comparison to the manual one ( $60.08^\circ \pm 14.72^\circ$  versus  $48.47^\circ \pm 7.67^\circ$ ;  $p < 0.0001$ ) (►Table 4).

Cases were categorized considering those presenting a glenoid inclination within the normal range (-10 to +10°) and those with anatomical variation of this parameter. For cases within the normal range, the vault method resulted in significantly higher values than the automated ( $p = 0.04$ ) and the Friedman et al.<sup>12</sup> methods ( $p = 0.0004$ ). Interestingly, for cases with a version higher than 10°, the mean version obtained with the automated method was significantly higher than that obtained with Friedman et al.<sup>12</sup> method ( $p = 0.001$ ), but similar to that obtained with vault method ( $p = 0.13$ ). The mean values for subluxation obtained with the automated method were significantly higher than those obtained with the manual method in both subgroups evaluated (►Table 5).

The cases were then categorized considering inclination, measured by the automated method. For cases with inclination



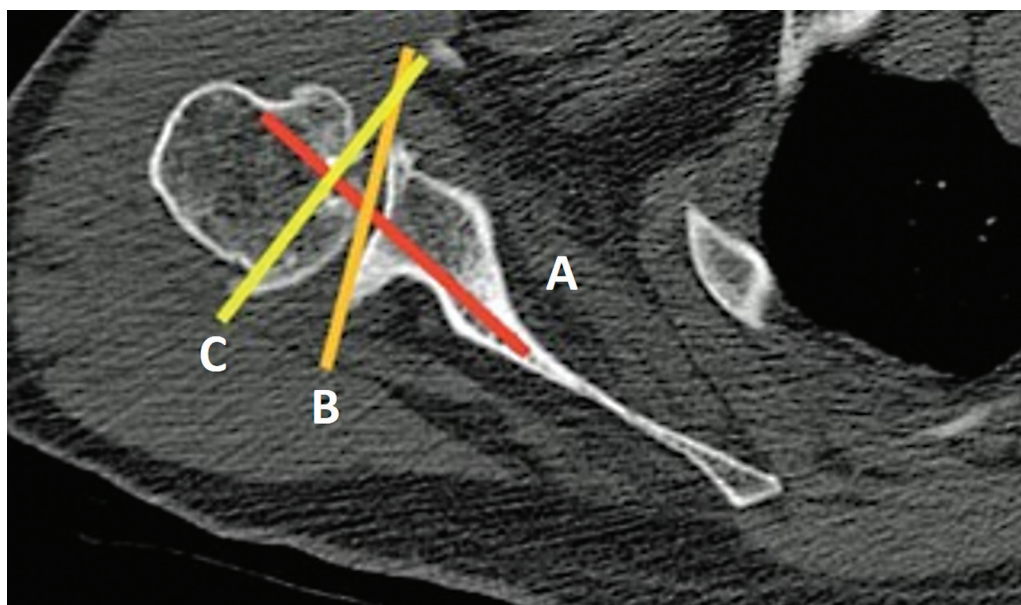

**Fig. 2** The vault method for the measurement of the version, which was defined in the axial section as a triangle composed of the anterior and posterior walls of the scapula neck and the glenoid articular surface. The angle is determined by the lines: (A) vault axis, (B) glenoid line, and (C) line perpendicular to the vault axis.


within the normal range, the mean version obtained with the vault method was significantly higher than that obtained with the Friedman et al.<sup>12</sup> method ( $p=0.1$ ), with no differences between the automated and the manual methods. For cases with inclination higher than  $10^\circ$ , the mean version was significantly underestimated by the Friedman et al.<sup>12</sup> in comparison to the automated ( $p=0.002$ ) and the vault methods ( $p=0.007$ ).

In cases within the normal range of inclination, this parameter was overestimated by the manual method in comparison to the automated one ( $p=0.001$ ). Regarding


subluxation, the mean values obtained with automated method were significantly higher than those obtained with the manual method in both subgroups evaluated ( $\rightarrow$  Table 6).

## Discussion


The success of shoulder arthroplasty depends on the proper positioning of the implant.<sup>1</sup> The surgeon's ability to identify morphological changes in the glenoid, especially regarding the version and inclination, is extremely important, as it

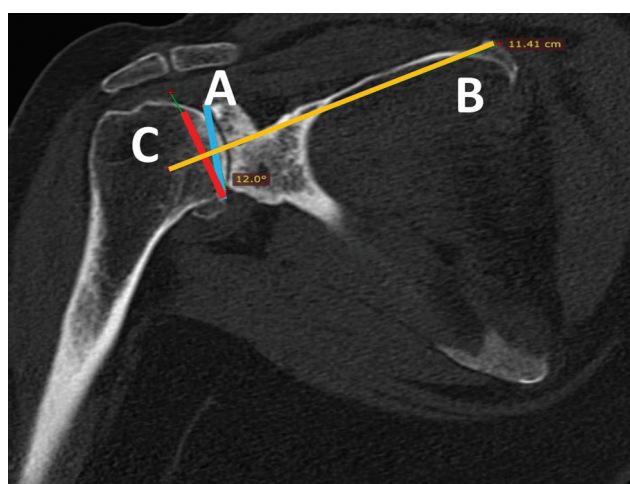

**Fig. 3** Maurer et al.<sup>14</sup> method for the measurement of the glenoid inclination, which was performed in the oblique coronal plane of the computed tomography scan, and the slice that best captured the floor of the supraspinatus fossa was selected. (A) Line tangent to the anterior and posterior edges of the glenoid, (B) supraspinatus fossa line, and (C) line perpendicular to line B determining the glenoid inclination.

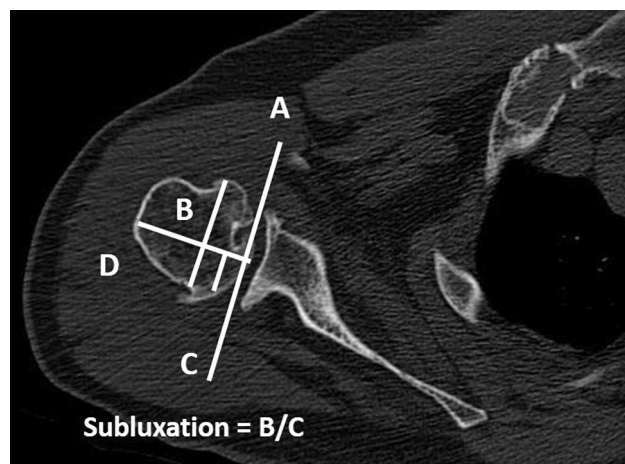

**Fig. 4** Walch et al.<sup>4</sup> method to determine humeral head subluxation. (A) Line tangent to the anterior and posterior edges of the glenoid, (B) line perpendicular to the face of the glenoid at its midpoint, (C) line parallel to line A, dividing the middle third of the humeral head, and (D) part of the humeral head posterior to the center of the glenoid. Subluxation index =  $D/C$ .

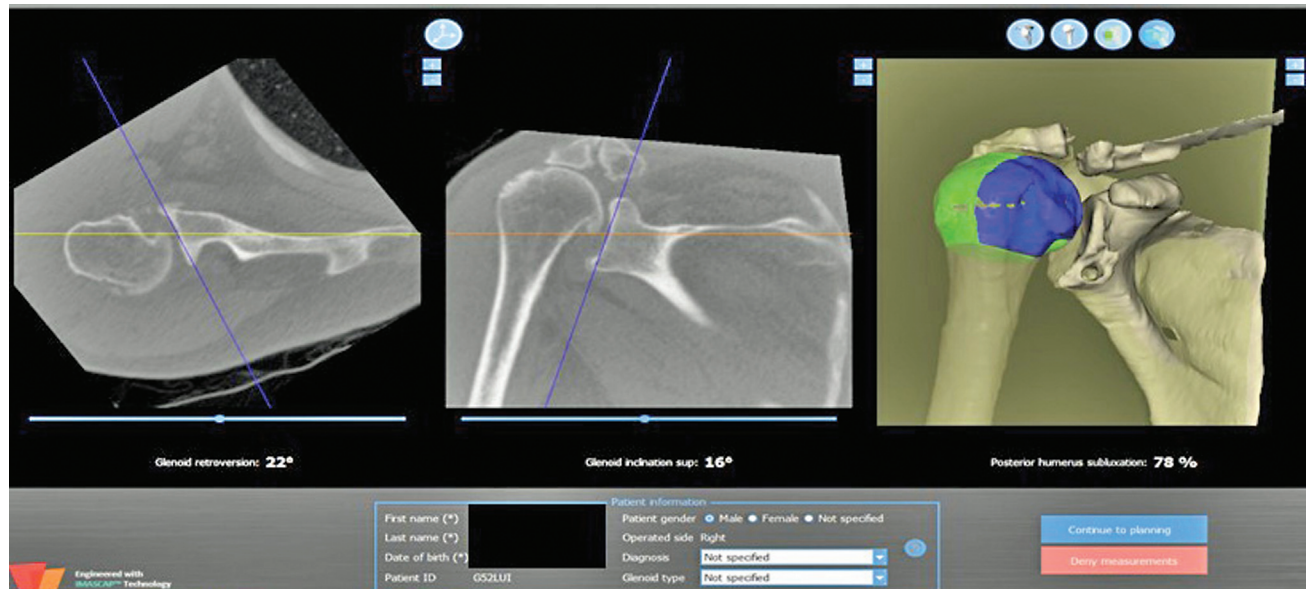

**Fig. 5** Initial screen of the Blueprint software showing the values of the glenoid version and inclination, and humeral head subluxation.

**Table 1** Interclass correlation coefficients for version, by the Friedman et al.<sup>12</sup> and vault methods, inclination, and subluxation

Variables	ICC	Inferior confidence interval	Superior confidence interval
Version according to the Friedman et al. <sup>12</sup> method	0.847	0.751	0.913
Version according to the vault method	0.845	0.744	0.931
Inclination	0.890	0.821	0.938
Subluxation	0.840	0.712	0.917

**Table 2** Version measurement

	Blueprint	Friedman et al. <sup>12</sup>	Vault
Version (mean $\pm$ standard deviation)	10.45° $\pm$ 7.1° <sup>a</sup>	8.07° $\pm$ 6.1° <sup>a, b</sup>	10.42° $\pm$ 6.2° <sup>b</sup>
Average difference (95% confidence interval)	–	2.37° (0.79–3.9°)	0.023° (–1.8–1.9°)
Maximum difference		11°	13.64°

Notes: <sup>a</sup> $p = 0.0059$ , Friedman et al.<sup>12</sup> test, Dunn posttest; <sup>b</sup> $p = 0.0005$ , Friedman et al.<sup>12</sup> test, Dunn posttest.

**Table 3** Number of cases in which the mean obtained by measurements using manual methods differed from automated measurements, stratified by degrees of difference

	Friedman et al. <sup>12</sup>	Vault
Difference $< 5^\circ$ in relation to the Blueprint software: n (%)	23 (60.5%)	21 (57.8%)
Difference of 5–10° in relation to the Blueprint software: n (%)	14 (36.8%)	13 (34.2%)
Difference $> 10^\circ$ in relation to the Blueprint software: n (%)	1 (2.6%)	3 (7.8%)

Notes: Chi-squared test;  $p = 0.57$ .

avoids misplacements that compromise the survival of the procedure.<sup>2,4,7</sup>

However, manual 2D methods to define glenoid morphology present limitations and inaccuracies because of the

difficulty in segmenting CT images in the anatomical plane of the scapula. The discrepancies motivated the development of automated programs for preoperative planning, whose use has become increasingly frequent in an effort to improve the

**Table 4** Measurement of inclination and sublaxation

	Blueprint	Manual	p
Inclination (mean ± standard deviation)	11.85° ± 9.8°	11.24° ± 5.44°	0.377
Sublaxation (mean ± standard deviation)	60.08° ± 14.72°	48.47° ± 7.67°	< 0.0001

Note: Wilcoxon Test.

**Table 5** Comparison regarding the mean version, inclination, and sublaxation using the automated and manual methods, categorized by version measured by the automated method

Version (°)		Parameter		p-value
<b>Version (°): mean ± standard deviation</b>				
	Blueprint	Friedman et al. <sup>12</sup>	Vault	
0–10 (n = 21)	5.6 ± 2.8 <sup>a</sup>	5.4 ± 4.0 <sup>b</sup>	7.7 ± 3.9 <sup>a, b</sup>	0.01*
> 10 (n = 17)	16.3 ± 6.5 <sup>c</sup>	11.3 ± 6.9 <sup>c</sup>	13.7 ± 7.0	0.0061*
<b>Inclination (°): mean ± standard deviation</b>				
	Blueprint	Manual		
0–10 (n = 21)	11.5 ± 11.5	10.9 ± 6.0		0.7 <sup>#</sup>
> 10 (n = 17)	10.8 ± 5.0	11.4 ± 4.8		0.5 <sup>#</sup>
<b>Sublaxation (°): mean ± standard deviation</b>				
	Blueprint	Manual		
0–10 (n = 21)	51.3 ± 10.4	45.7 ± 7.2		0.005 <sup>#</sup>
> 10 (n = 17)	69.8 ± 12.5	52.0 ± 7.1		< 0.0001 <sup>#</sup>

Notes: \*One-way analysis of variance (ANOVA); <sup>a</sup>p = 0.04; <sup>b</sup>p = 0.0004; <sup>c</sup>p = 0.001; Tukey multiple comparisons test; <sup>#</sup>t-test.

**Table 6** Comparison regarding the mean of the inclination using the automated and manual methods, categorized by the severity of the inclination measured by the automated method

Inclination (°)		Parameter		p-value
<b>Version (°): mean ± standard deviation</b>				
	Blueprint	Friedman et al. <sup>12</sup>	Vault	
0–10 (n = 21)	8.9 ± 6.4	8.3 ± 6.2 <sup>a</sup>	10.9 ± 7.3 <sup>a</sup>	0.03*
> 10 (n = 17)	12.3 ± 7.8 <sup>b</sup>	7.7 ± 6.3 <sup>b, c</sup>	9.7 ± 4.8 <sup>c</sup>	0.003*
<b>Inclination (°): mean ± standard deviation</b>				
	Blueprint	Manual		
0–10 (n = 21)	5.9 ± 2.9	8.7 ± 3.8		0.001 <sup>#</sup>
> 10 (n = 17)	17.6 ± 9.9	14.0 ± 5.8		0.1 <sup>#</sup>
<b>Sublaxation (°): mean ± standard deviation</b>				
	Blueprint	Manual		
0–10 (n = 21)	60.33 ± 15.0	49.9 ± 6.8		0.0001 <sup>#</sup>
> 10 (n = 17)	58.7 ± 14.5	46.8 ± 8.6		0.000 <sup>#</sup>

Notes: \*One-way analysis of variance (ANOVA); <sup>a</sup>p = 0.01; <sup>b</sup>p = 0.002; <sup>c</sup>p = 0.007; Tukey multiple comparisons test; <sup>#</sup>t-test.

understanding of the anatomy and the subsequent positioning and fixation of the prosthetic components.<sup>8,9</sup> However, its routine use still does not occur in the practice of most surgeons who perform shoulder arthroplasties.<sup>8,18–20</sup> Moreover, there are controversies regarding the accuracy of these methods and the ideal placement of the implants.<sup>21–25</sup>

In the clinical practice at low- and middle-income countries, 2D CT images unformatted in the plane of the scapula

are broadly used, which, despite representing a limitation, is a reality. In the present study, manual measurements of the version, by both the Friedman et al.<sup>12</sup> and vault methods, as well as inclination and sublaxation, showed a good ICC. Interestingly, other studies<sup>5,6,9,10</sup> have shown that the version of the glenoid measured on 2D CT images presents significant interobserver variability due to the variation in the coronal and sagittal rotation of the scapula in relation to

the patient's position on the examination table. However, in the present study, we obtained a good ICC, which we attribute to the fact that all evaluators are shoulder surgeons with more than five years of training and with experience in performing shoulder arthroplasties.

In the present study, the mean glenoid version measured through the automated method was similar to that obtained through the vault method. However, the version measured by the Friedman et al.<sup>12</sup> method was lower than that obtained by the automated and vault methods. Still, based on the comparisons of the versions, only 1 case showed a difference greater than 10° when comparing the Friedman et al.<sup>12</sup> method with the automated method. Therefore, it was shown that the Friedman et al.<sup>12</sup> method is less accurate than the vault method when the automated method was used as a standard. In 2014, Matsumara et al.<sup>13</sup> compared the measurement of the version by the Friedman et al.<sup>12</sup> and vault methods and, similarly, stated that both methods present good interobserver agreement, but that the vault method enables an easier measurement, since it does not depend on the anatomical variations of the body of the scapula or its inclusion in the exam.<sup>11,13,15,23</sup>

Remarkably, using the automated method as a standard, in cases in which the version was within the normal range, we did not observe significant differences between the automated and Friedman et al.<sup>12</sup> methods; however, in cases in which the version was out of the normal range (> 10°), the mean version obtained by the Friedman et al.<sup>12</sup> method was significantly lower than that obtained by the automated method. Altogether, these results enable us to conclude that the use of version measurement by the automated method is more important in cases in which deformities on the glenoid surface are more severe, possibly influencing the clinical practice, both in the correction of the version and in the correct positioning of the implant. This finding is compatible with that found in the literature, in which Chalmers et al.<sup>26</sup> demonstrated that, in deformities classified as B2 using the morphological classification proposed by Walch et al.,<sup>4</sup> the measurement of the version by CT images is superior.<sup>26,27</sup>

In a recent study, Reid et al.<sup>28</sup> found results similar to ours, showing that the measurement of the version in 2D CT scans, using the Friedman et al.<sup>12</sup> method, presents both high intra- and interclass correlation rates. On the other hand, this study<sup>28</sup> also found significant differences between measurements using manual and automated methods. However, when the cases were categorized according to version severity, the authors<sup>28</sup> did not find differences between the methods in the different subgroups evaluated, suggesting that the version magnitude does not influence the differences between the methods. This result contrasts with the findings of the present study, as we found that the manual method underestimated glenoid inclination, in comparison to automated method, in cases with a version greater than 10°. The different version ranges used to stratify the cases and the different diagnosis included in our series may explain these differences.

Glenoid inclination presented similar values when assessed by the manual or automated methods. Iannotti et al.,<sup>21</sup> regarding inclination measurements on formatted CT scans, observed that there were no differences from those obtained with the automated method. In relation to unformatted images, an expressive difference was found. In 94% of the cases, the difference in inclination between the unformatted and the formatted images was greater than 5°, again a value with significance in the clinical practice.<sup>21</sup> In our series, when the cases were categorized according to severity of the inclination, differences were found in the measurement of mild cases (0–10° of inclination), in which the manual method resulted in a mean that was significantly higher than that obtained by the automated method ( $p = 0.001$ ). In a study published in 2020, Choi et al.<sup>29</sup> compared inclination measured by automated and 2D methods and found that the 3D method resulted in measurements that were significantly lower than those obtained with the 2D method. Although the authors<sup>29</sup> did not perform a subgroup analysis, the data evaluated presented mean values for version and inclination compatible with the cases included in the subgroup of mild cases of the present study.

In relation to subluxation, significant differences were found between the manual and automated methods. Other studies<sup>30</sup> have already reported an error intrinsic to the measurement of subluxation using the Walch et al.<sup>4</sup> method. The subluxation index, described by Walch et al.,<sup>4</sup> is measured on a CT transverse cut. The scapular body has an inclination compared to the body of the patient in whom the CT cross-sections are aligned, which leads to errors in the 2D CT measurements.<sup>5,10,11,26,27,30</sup> Jacxsens et al.<sup>30</sup> concluded that measurements based on shoulders reconstructed in 3D seem to be more appropriate, as they reconstruct the bone anatomy regardless of the patient's orientation at the time of the exam, and could be, therefore, another more reliable measurement than the 2D one, which is underestimated.

An interesting finding of the present study was that the differences between the subluxation measurements obtained by the automated and manual methods tended to increase with the severity of the version, suggesting that the greater the version angle, the more the manual method underestimates the measurement of the subluxation, when the automated method is used as the default. Further studies are needed to assess the clinical impact of such a finding, once it can directly impact on surgical planning.

Chalmers et al.<sup>26</sup> evaluated the glenoid version and inclination and humeral head subluxation values using corrected and uncorrected CT scans, and compared these measurements with the values provided by the Blueprint software. They<sup>26</sup> concluded that the orientation of the slices of CT scans formatted in the plane of the scapula presented a decrease in retroversion measurements compared to unformatted CT scans. On the other hand, the authors<sup>26</sup> verified that there are no differences between unformatted CT scans and the values of automated programs. In 48% of the cases, the difference between the uncorrected and corrected versions was greater than 5°, which is considered significant in the



clinical practice.<sup>21</sup> These findings are similar to the results obtained in our series.

Shukla et al.<sup>23</sup> used the same automated program used in the present study and found similar results between the manual and automated methods for the measurements of version and inclination, but with an important difference in the percentage measurements of subluxation of the humeral head. Thus, like these authors,<sup>23</sup> we believe that measuring the percentage of subluxation is essential in the preoperative planning of shoulder arthroplasty, and that such variability in the values of this parameter between the manual and automated methods should be taken into consideration, since the percentage of posterior head subluxation is a radiographic criterion that influences the surgical technique to be used and the selection of implants and manual measurements of this parameter are underestimated by the manual method.

As a limitation of the present study, we used a single automated preoperative planning program. We understand that these programs present a variability of measurements among them, since they use different anatomical parameters to format the images.

## Conclusion

The manual method is effective in measuring the glenoid version and inclination when performed by experienced surgeons, and the vault method is more accurate than the Friedman et al.<sup>12</sup> method in patients with glenoids with greater deformities. However, the measurement of the percentage of posterior subluxation of the humeral head presents a great discrepancy between the manual and automated methods. Such differences underscore the need for further studies that aim to assess the impact of such differences on the outcome of procedures, since several uncertainties exist regarding the accuracy of manual and automated methods and the selection and correct positioning of the implants.

### Financial Support

The authors declare that they have received no financial support from agencies in the public, private, or non-profit sectors to conduct the present study.

### Conflict of Interests

The authors have no conflict of interests to declare.

## References

- Walch G, Mesiha M, Boileau P, et al. Three-dimensional assessment of the dimensions of the osteoarthritic glenoid. *Bone Joint J* 2013;95-B(10):1377–1382
- Shapiro TA, McGarry MH, Gupta R, Lee YS, Lee TQ. Biomechanical effects of glenoid retroversion in total shoulder arthroplasty. *J Shoulder Elbow Surg* 2007;16(3, Suppl):S90–S95
- Iannotti JP, Greeson C, Downing D, Sabesan V, Bryan JA. Effect of glenoid deformity on glenoid component placement in primary shoulder arthroplasty. *J Shoulder Elbow Surg* 2012;21(01):48–55
- Walch G, Badet R, Boulahia A, Khoury A. Morphologic study of the glenoid in primary glenohumeral osteoarthritis. *J Arthroplasty* 1999;14(06):756–760
- Ganapathi A, McCarron JA, Chen X, Iannotti JP. Predicting normal glenoid version from the pathologic scapula: a comparison of 4 methods in 2- and 3-dimensional models. *J Shoulder Elbow Surg* 2011;20(02):234–244
- Hoenecke HR Jr, Hermida JC, Flores-Hernandez C, D'Lima DD. Accuracy of CT-based measurements of glenoid version for total shoulder arthroplasty. *J Shoulder Elbow Surg* 2010;19(02):166–171
- Scalise JJ, Bryan J, Polster J, Brems JJ, Iannotti JP. Quantitative analysis of glenoid bone loss in osteoarthritis using three-dimensional computed tomography scans. *J Shoulder Elbow Surg* 2008;17(02):328–335
- Iannotti J, Baker J, Rodriguez E, et al. Three-dimensional preoperative planning software and a novel information transfer technology improve glenoid component positioning. *J Bone Joint Surg Am* 2014;96(09):e71
- Boileau P, Cheval D, Gauci MO, Holzer N, Chaoui J, Walch G. Automated Three-Dimensional Measurement of Glenoid Version and Inclination in Arthritic Shoulders. *J Bone Joint Surg Am* 2018;100(01):57–65
- Gross DJ, Golijanin P, Dumont GD, et al. The effect of sagittal rotation of the glenoid on axial glenoid width and glenoid version in computed tomography scan imaging. *J Shoulder Elbow Surg* 2016;25(01):61–68
- Lewis GS, Armstrong AD. Glenoid spherical orientation and version. *J Shoulder Elbow Surg* 2011;20(01):3–11
- Friedman RJ, Hawthorne KB, Genez BM. The use of computerized tomography in the measurement of glenoid version. *J Bone Joint Surg Am* 1992;74(07):1032–1037
- Matsumura N, Ogawa K, Ikegami H, Collin P, Walch G, Toyama Y. Computed tomography measurement of glenoid vault version as an alternative measuring method for glenoid version. *J Orthop Surg Res* 2014;9(01):17
- Maurer A, Fucetese SF, Pfirrmann CW, et al. Assessment of glenoid inclination on routine clinical radiographs and computed tomography examinations of the shoulder. *J Shoulder Elbow Surg* 2012;21(08):1096–1103
- RadiAnt® DICOM Viewer, Poznan, Poland. Available from: [www.radiantviewer.com/pt-br](http://www.radiantviewer.com/pt-br)
- van de Bunt F, Pearl ML, Lee EK, Peng L, Didomenico P. Glenoid version by CT scan: an analysis of clinical measurement error and introduction of a protocol to reduce variability. *Skeletal Radiol* 2015;44(11):1627–1635
- Favard L, Berhouet J, Walch G, Chaoui J, Lévine C. Superior glenoid inclination and glenoid bone loss: Definition, assessment, biomechanical consequences, and surgical options. *Orthopade* 2017;46(12):1015–1021
- Werner BS, Hudek R, Burkhart KJ, Gohlke F. The influence of three-dimensional planning on decision-making in total shoulder arthroplasty. *J Shoulder Elbow Surg* 2017;26(08):1477–1483
- Rosenthal Y, Rettig SA, Virk MS, Zuckerman JD. Impact of preoperative 3-dimensional planning and intraoperative navigation of shoulder arthroplasty on implant selection and operative time: a single surgeon's experience. *J Shoulder Elbow Surg* 2020;29(12):2564–2570
- Hartzler RU, Denard PJ, Griffin JW, Werner BC, Romeo AA. Surgeon acceptance of an initial 3D glenoid preoperative plan: rates and risk factors. *J Shoulder Elbow Surg* 2021;30(04):787–794
- Iannotti JP, Walker K, Rodriguez E, Patterson TE, Jun BJ, Ricchetti ET. Accuracy of 3-Dimensional Planning, Implant Templating, and Patient-Specific Instrumentation in Anatomic Total Shoulder Arthroplasty. *J Bone Joint Surg Am* 2019;101(05):446–457
- Berhouet J, Jacquot A, Walch G, Deransart P, Favard L, Gauci MO. Preoperative planning of baseplate position in reverse shoulder



- arthroplasty: Still no consensus on lateralization, version and inclination. *Orthop Traumatol Surg Res* 2022;108(03):103115
- 23 Shukla DR, McLaughlin RJ, Lee J, Nguyen NTV, Sanchez-Sotelo J. Automated three-dimensional measurements of version, inclination, and subluxation. *Shoulder Elbow* 2020;12(01):31–37
  - 24 Raiss P, Walch G, Wittmann T, Athwal GS. Is preoperative planning effective for intraoperative glenoid implant size and type selection during anatomic and reverse shoulder arthroplasty? *J Shoulder Elbow Surg* 2020;29(10):2123–2127
  - 25 Denard PJ, Provencher MT, Lädermann A, Romeo AA, Parsons BO, Dines JS. Version and inclination obtained with 3-dimensional planning in total shoulder arthroplasty: do different programs produce the same results? *JSES Open Access* 2018;2(04):200–204
  - 26 Chalmers PN, Salazar D, Chamberlain A, Keener JD. Radiographic characterization of the B2 glenoid: the effect of computed tomographic axis orientation. *J Shoulder Elbow Surg* 2017;26(02):258–264
  - 27 Bercik MJ, Kruse K II, Yalozis M, Gauci MO, Chaoui J, Walch G. A modification to the Walch classification of the glenoid in primary glenohumeral osteoarthritis using three-dimensional imaging. *J Shoulder Elbow Surg* 2016;25(10):1601–1606
  - 28 Reid JJ, Kunkle BF, Greene AT, Eichinger JK, Friedman RJ. Variability and reliability of 2-dimensional vs. 3-dimensional glenoid version measurements with 3-dimensional preoperative planning software. *J Shoulder Elbow Surg* 2022;31(02):302–309
  - 29 Choi CH, Kim HC, Kang D, Kim JY. Comparative study of glenoid version and inclination using two-dimensional images from computed tomography and three-dimensional reconstructed bone models. *Clin Shoulder Elbow* 2020;23(03):119–124
  - 30 Jacxsens M, Van Tongel A, Willemot LB, Mueller AM, Valderrabano V, De Wilde L. Accuracy of the glenohumeral subluxation index in nonpathologic shoulders. *J Shoulder Elbow Surg* 2015;24(04):541–546