

Percutaneous Chemotherapy Port-A-Cath Shortening Technique

Arta Kasaeian¹  Julio Calderon¹ Zubin Irani² Mohammad Ghasemi-Rad¹ 

¹Division of Vascular and Interventional Radiology, Department of Radiology, Baylor College of Medicine, Houston, Texas, United States

²Division of Vascular and Interventional Radiology, Department of Radiology, Massachusetts General Hospital, Harvard Medical School, Boston, Massachusetts, United States

Address for correspondence Mohammad Ghasemi-Rad, MD, Division of Vascular and Interventional Radiology, Department of Radiology, Baylor College of Medicine, 3707 Bellefontaine St, Houston, TX 77025, United States (e-mail: mdghrad@gmail.com).

Arab J Intervent Radiol

Introduction

Central venous chest ports are typically implanted as long-term points of vascular access for cancer patients for the administration of chemotherapy.¹ Correct positioning of the tip is important to ensure appropriate function and to avoid complications such as venous perforation, thrombosis, arrhythmias, retrograde injection, and overall dysfunction of the port. Malposition of the catheter tip may occur due to improper initial placement or changes such as weight loss, as seen with the progression of many types of cancer. This report provides additional support for the percutaneous

shortening of port-a-cath and expands on technique and outcomes.^{2,3}

Technique

A retrospective review to identify three patients who underwent percutaneous port catheter tip shortening. The technique used was the same for all cases (→ **Fig. 1A** and **B**). The right neck and upper chest area was prepped and draped in the standard sterile manner. Under ultrasound guidance, access to the right internal jugular vein was obtained and was then upsized for an 8-F, 4-cm vascular sheath (Merit



Fig. 1 (A and B) Preprocedure computed tomography (CT) chest coronal and preprocedural saved fluoroscopic image in an incidentally found port-a-cath in the lower right atrium/ventricle.

DOI <https://doi.org/10.1055/s-0044-1787788>.
ISSN 2542-7075.

© 2024. The Author(s).

This is an open access article published by Thieme under the terms of the Creative Commons Attribution License, permitting unrestricted use, distribution, and reproduction so long as the original work is properly cited. (<https://creativecommons.org/licenses/by/4.0/>)

Thieme Medical and Scientific Publishers Pvt. Ltd., A-12, 2nd Floor, Sector 2, Noida-201301 UP, India




Fig. 2 Picture of right neck showing externalization of port-a-cath.

Medical, Utah, United States). A 15-mm Amplatz Goose Neck snare (Medtronic, Minnesota, United States) was used to engage the distal end of the port-a-cath tubing, which was then externalized (►Figs. 2 and 3). The appropriate length




Fig. 3 Drawing demonstrating how the catheter was snared, and externalized following by shortening.

was calculated based on initial chest radiograph in inspiratory phase. The catheter tubing was trimmed to the length and the catheter was repositioned in the lower superior vena cava or cavoarterial junction (►Fig. 4A and B). Access to the port was established, confirming free blood flow through the flushing of contrast. The port was then instilled with 2 mL of heparin.

Discussion

Current standard for central venous port catheter revision is surgical and involves excision of the port pocket which increases the risk of infections and pain at the incision site.⁴ The new port is either placed in the same pocket or anew on the same or contralateral chest. The described technique for percutaneous endovascular port revision is effective at shortening too-long central venous catheter port tips and bypasses the surgical complications of the traditional methods. Percutaneous endovascular port revision provides a faster and safer technique performed through a single vascular puncture site at the neck, which most likely proves more comfortable to the patient given the lack of need for an incision.^{2,3}

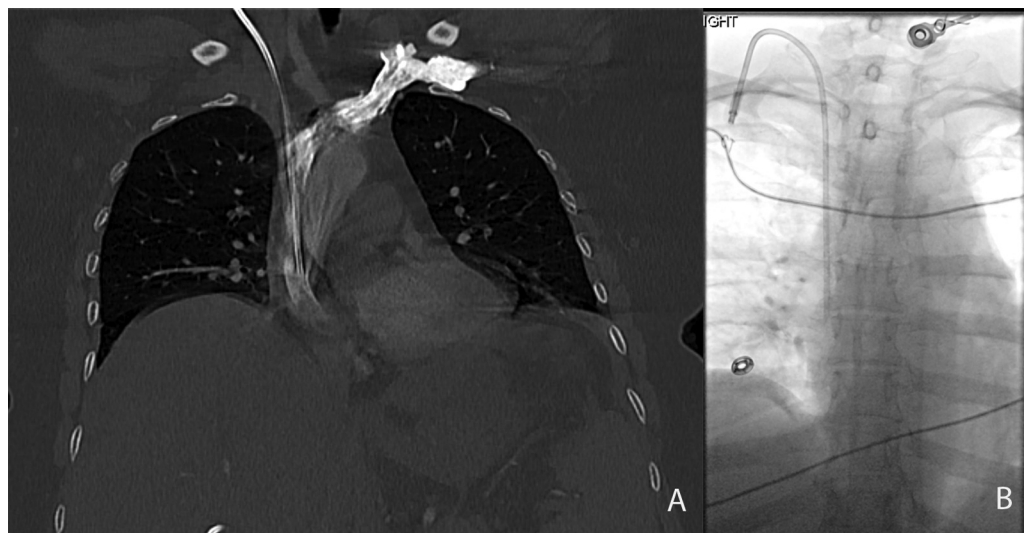


Fig. 4 (A and B) Postprocedural computed tomography (CT) chest coronal and fluoroscopic image shows port tip in the lower superior vena cava (SVC).

Conflict of Interest

None declared.

References

- 1 Kim HJ, Yun J, Kim HJ, et al. Safety and effectiveness of central venous catheterization in patients with cancer: prospective observational study. *J Korean Med Sci* 2010;25(12):1748–1753
- 2 Duncan C, Trerotola SO. Outcomes of a percutaneous technique for shortening of totally implanted indwelling central venous chest port catheters. *J Vasc Interv Radiol* 2016;27(07):1034–1037
- 3 Murthy R, Arbabzadeh M, Richard H III, Levitin A, Lund G, Stainken B. Endovascular technique for revision of excess catheter length in subcutaneous implanted venous access devices. *Cardiovasc Intervent Radiol* 2004;27(03):259–261
- 4 Erdemir A, Rasa HK. Impact of central venous port implantation method and access choice on outcomes. *World J Clin Cases* 2023; 11(01):116–126